


Lab name: SRI Instruments  
 Client: Puro/Guy  
 Client ID: N11853  
 Analysis date: 03/03/2021 16:59:13  
 Method: Heated Inj Restek Liner 200C  
 Description: FID 300C  
 Column: 30MXT502  
 Carrier: H2 from BIHG  
 Integration: Peak sens=80.0 Base sens=10.0 Min area= 1.00 Standard=100.000 Sample=100.000 Tangents=off  
 Data file: Puro489.chr ()  
 Sample: 333NG/UL NO is

Temperature program:

Init temp	Hold	Ramp	Final temp
20.00	10.000	0.000	50.00

Events:

Time	Event
0.000	ZERO
0.500	INTEG IMMEDIATE
4.000	INTEG IMMEDIATE

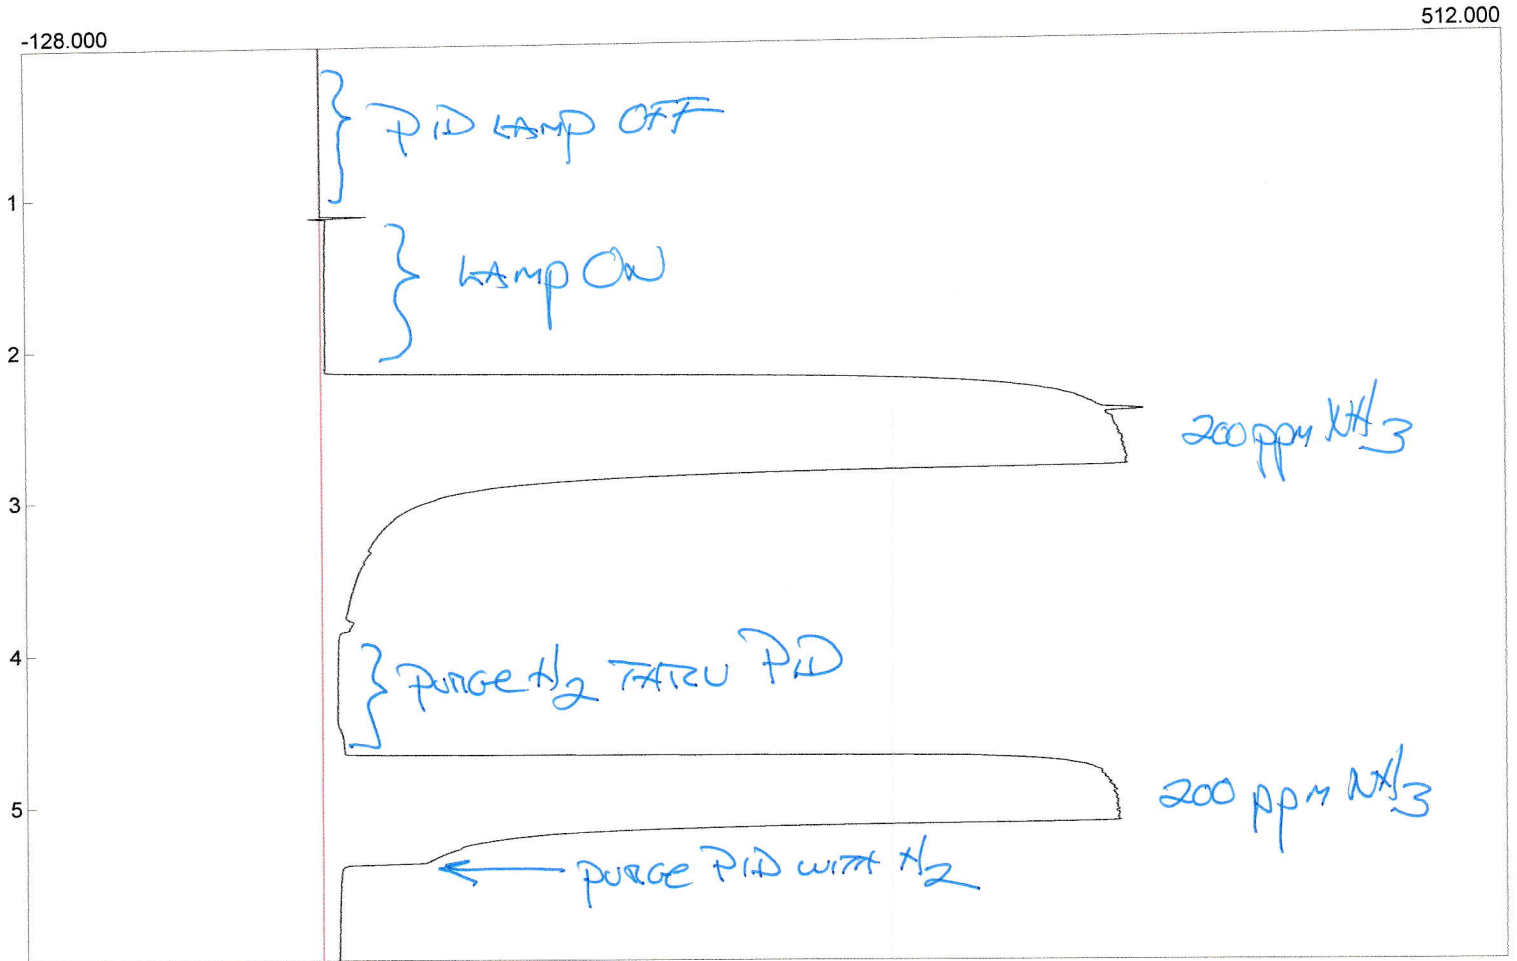

Component	Retention	Area	Internal	Units
		0.0000	0.0000	