


Lab name: SRI Instruments  
 Client: Techno  
 Client ID: N11812  
 Analysis date: 06/16/2020 14:13:12  
 Method: syringe on-column  
 Description: RGD 287C  
 Column: 6' MS13X  
 Carrier: Helium@15psi=20ml/min  
 Data file: ARB188.chr ()  
 Sample: 5ul 1% mix

Temperature program:

Init temp	Hold	Ramp	Final temp
50.00	2.000	20.000	150.00
30.00	2.000	20.000	50.00

Events:

Time	Event
0.000	ZERO 100
1.000	INTEG IMMEDIATE

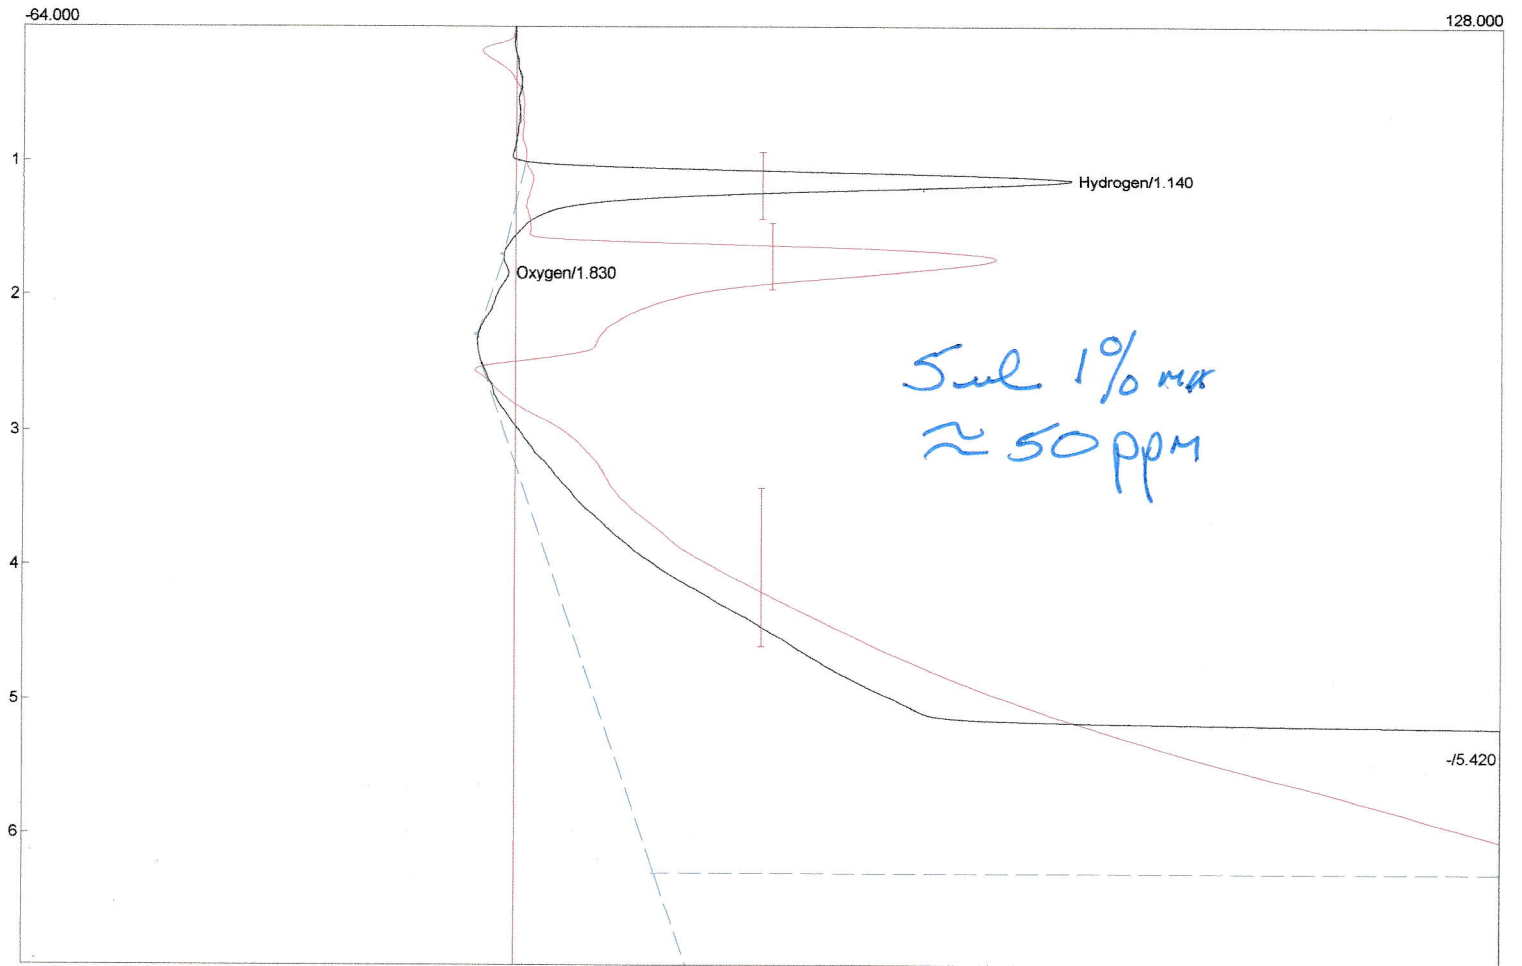

Component	Retention	Area	Internal	Units
Hydrogen	1.140	755.3466	50.0000	ppm
Oxygen	1.830	22.0720	0.0000	ppm
		777.4186	50.0000	


Lab name: SRI Instruments  
 Client: Techno  
 Client ID: N11812  
 Analysis date: 06/16/2020 12:50:36  
 Method: syringe on-column  
 Description: RGD 287C  
 Column: 6' MS13X  
 Carrier: Helium@15psi=20ml/min  
 Data file: ARB184.chr ()  
 Sample: .5ml room air

Temperature program:

Init temp	Hold	Ramp	Final temp
50.00	2.000	20.000	150.00
30.00	2.000	20.000	50.00

Events:

Time	Event
0.000	ZERO 100
1.000	INTEG IMMEDIATE

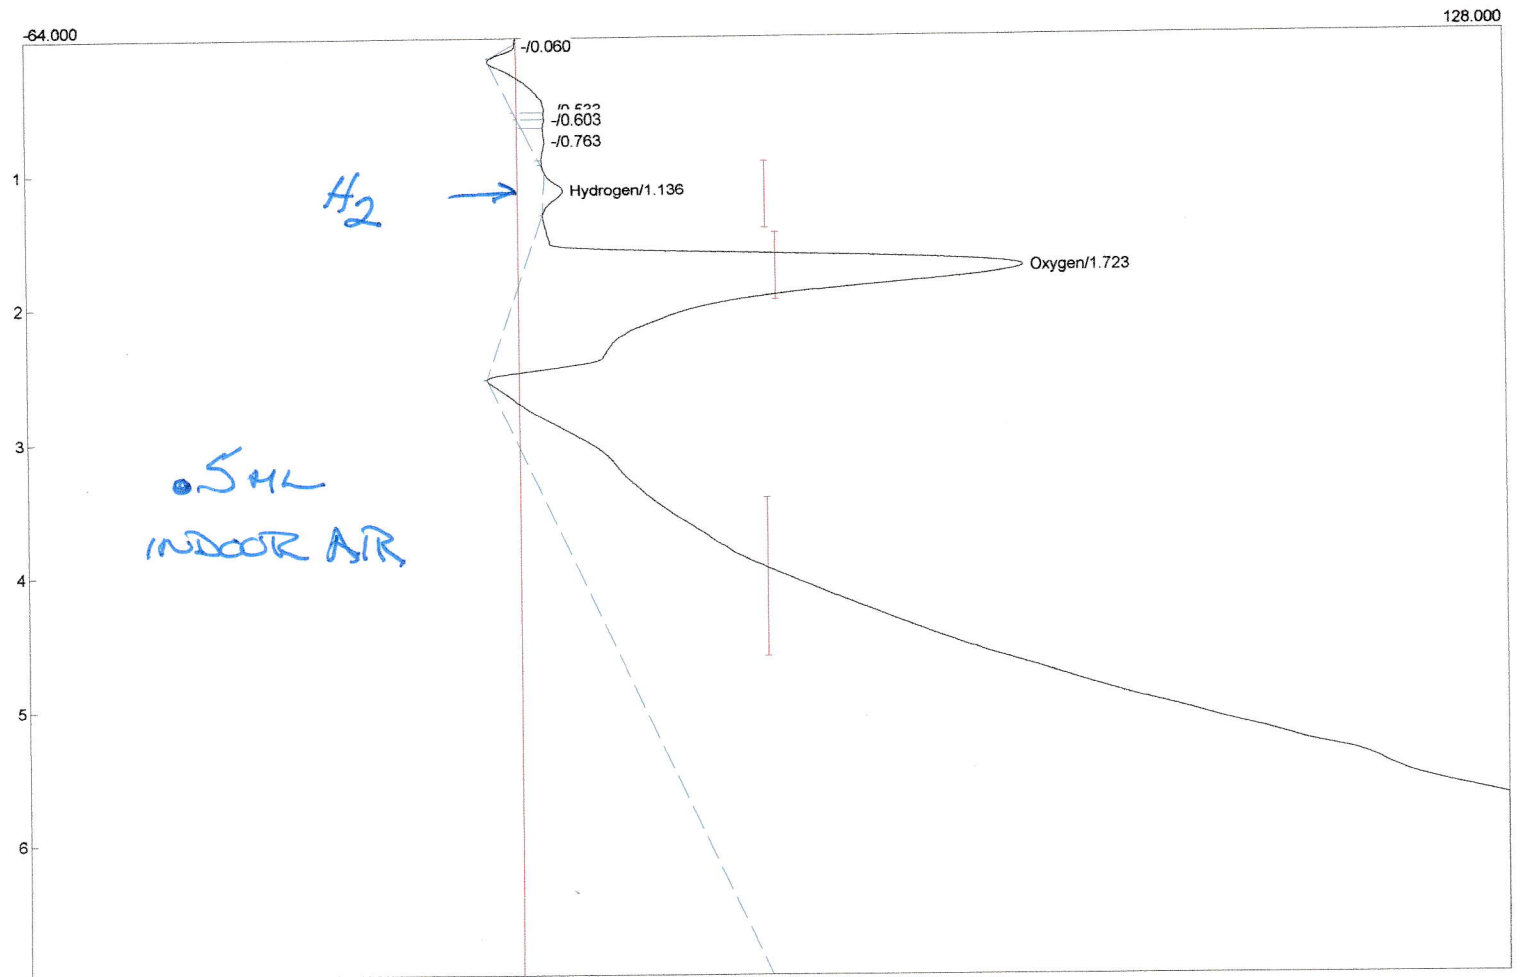

Component	Retention	Area	Internal	Units
Hydrogen	1.136	22.1742	3.8466	ppm
Oxygen	1.723	1631.6739	0.0000	ppm
		1653.8481	3.8466	


Lab name: SRI Instruments  
 Client: Techno  
 Client ID: N11812  
 Analysis date: 06/16/2020 13:16:02  
 Method: syringe on-column  
 Description: RGD 287C  
 Column: 6' MS13X  
 Carrier: Helium@15psi=20ml/min  
 Data file: ARB185.chr ()  
 Sample: .5ml outside air

Temperature program:

Init temp	Hold	Ramp	Final temp
50.00	2.000	20.000	150.00
30.00	2.000	20.000	50.00

Events:

Time	Event
0.000	ZERO 100
1.000	INTEG IMMEDIATE

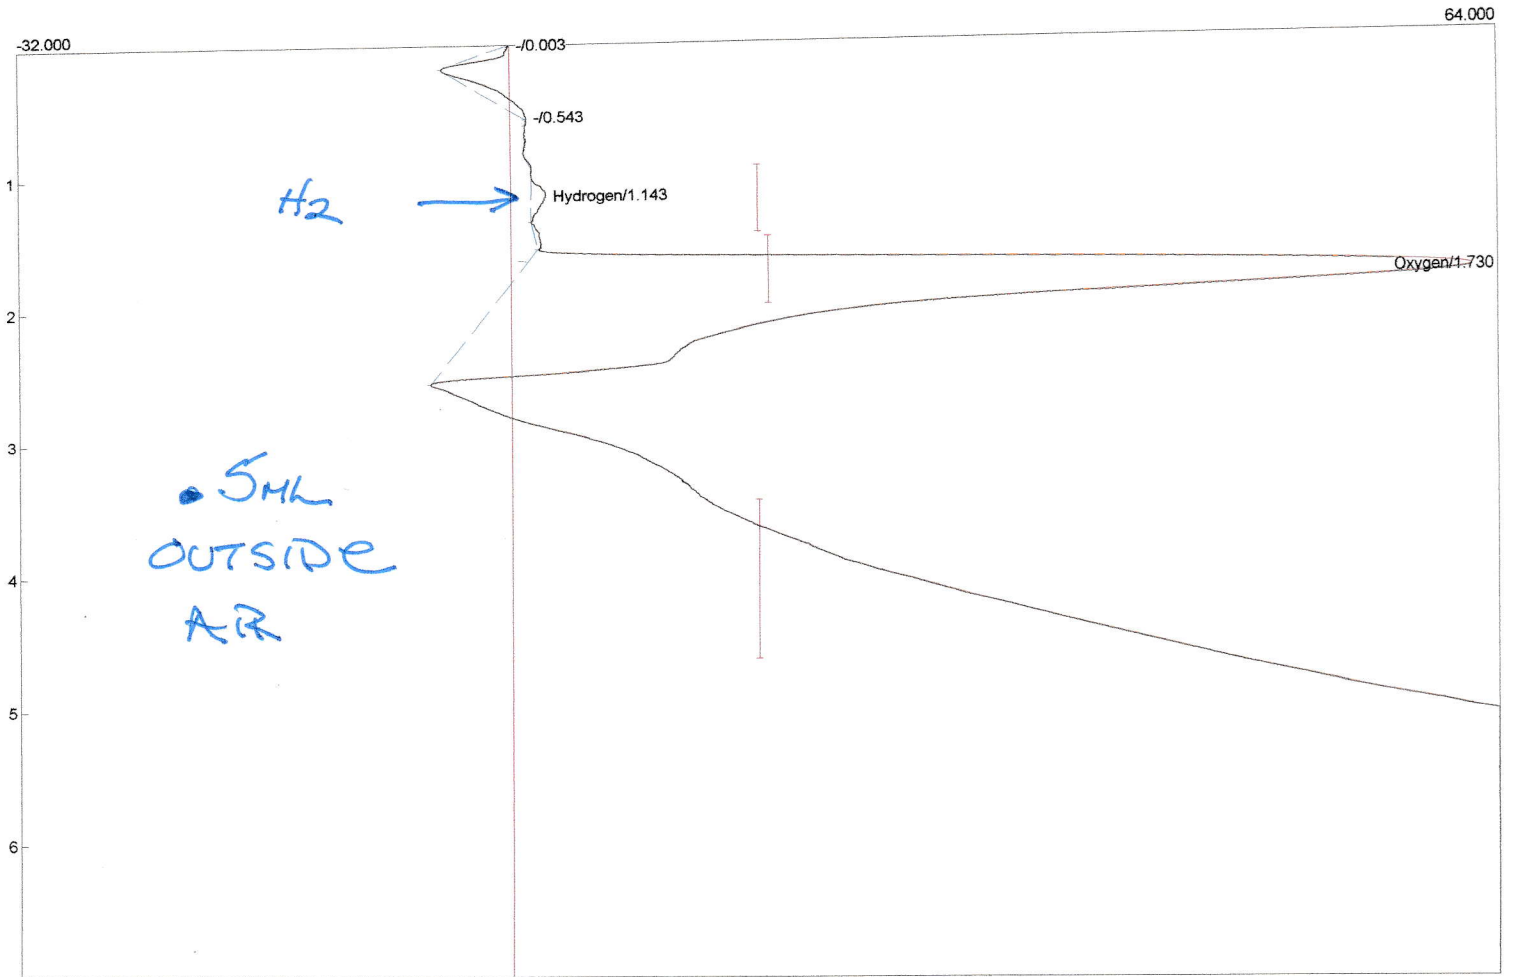

Component	Retention	Area	Internal	Units
Hydrogen	1.143	9.8259	1.7045	ppm
Oxygen	1.730	1528.2176	0.0000	ppm
		1538.0435	1.7045	